

Key Comparison COOMET.QM-K120

“Carbon dioxide in Air at urban level (480- 800) $\mu\text{mol/mol}$ ”

Final report

L. Konopelko¹, A.Kolobova¹, I.Chubchenko¹, O. Efremova¹, M. Rozhnov², D. Melnyk², S. Kisel², O. Levbarg², S. Shpilnyi², S. Yakubov², A. Mironchik³, V. Aleksandrov⁴, F. M. Kai⁵, T. Y. Wu⁵, J. Fang⁵, Y. Cui⁵, J. Mou⁵, W. Liu⁵.

¹*D.I.Mendeleev Institute for Metrology, 19, Moskovsky pr., St-Petersburg, 190005, Russia.*

²*All-Ukrainian State Research and Production Center of Standardization, Metrology, Certification and Consumers Rights Protection, 4, Metrologicheskaya str., Kiev, 03143, Ukraine.*

³*Belorussian State Institute for Metrology, Section for physico-chemical and optical measurements, sector for standards and gas mixtures, 8, Serova st., Minsk, Belarus.*

⁴*Kazakhstan Institute of Metrology, Karaganda branch, 22/2, Angerskaya st., Karaganda, 100009, Kazakhstan, Angerskayast. 22/2.*

⁵*National Metrology Centre (NMC), Agency for Science, Technology and Research (A*STAR), 1 Science Park Drive, 118221, Singapore.*

Field

Amount of substance

Subject

Comparison of carbon dioxide in air urban level (track A – core competences)

Table of contents

| | |
|--|----|
| Field | 1 |
| Subject | 1 |
| Table of contents | 1 |
| 1 Introduction | 2 |
| 2 Design and organization of comparison | 2 |
| 2.1 Participants | 2 |
| 2.2 Measurement standards..... | 2 |
| 2.3 The schedule..... | 4 |
| 3 Comparison measurements..... | 4 |
| 3.1 Control mixture..... | 4 |
| 3.2 Instrumentation and measurement procedure..... | 4 |
| 3.3 Stability measurements by participants..... | 6 |
| 3.4 Degrees of equivalence..... | 6 |
| 4 Results | 7 |
| 5 Supported CMC claims | 10 |
| 6 Discussion and conclusions | 10 |
| 7 References | 10 |
| Annex A – Measurement reports from participants..... | 11 |
| Measurement report from BELGIM..... | 12 |
| Measurement report from KAZINMETR | 18 |
| Measurement report from NMC, A*STAR (1)..... | 21 |
| Measurement report from NMC, A*STAR (2)..... | 25 |
| Measurement report from Ukrmetrteststandard | 29 |
| Measurement report from VNIIM..... | 35 |

1 Introduction

COOMET key comparison COOMET.QM-K120 is designed as linking to the appropriate CCQM comparison - CCQM-K120.b (2016-2018, Flores et al. 2018, [1]) and is intended to support CMCs of National Metrological Institutes of the countries – mainly members of COOMET.

The CCQM-K120.b was a gravimetric comparison which evaluated the level of compatibility of NMI preparative capabilities for carbon dioxide in air primary reference mixtures in the range (480-800) $\mu\text{mol/mol}$.

CCQM-K120.b is considered as a Track A comparison and tests core skills and competencies required in gravimetric preparation, analytical certification and purity analysis. Participants successful in CCQM-K120.b and the linked COOMET.QM-K120 comparison may use their results in the flexible scheme and underpin claims for all core mixtures in accordance with the GAWG strategy document [2].

2 Design and organization of comparison

2.1 Participants

Table 1 lists the participants of the comparison.

Table 1: List of participants

| Acronym | Country | Institute |
|--------------------------|---------|--|
| VNIIM (Pilot lab.) | RU | D.I.Mendeleyev Institute for Metrology, St-Petersburg, Russia |
| Ukrmetrt- eststandart | UA | All-Ukrainian State Research and Production Center of Standardization, Metrology, Certification and Consumers Rights Protection, Kiev, Ukraine |
| BelGIM | BY | Belorussian State Institute for Metrology, Minsk, Belarus |
| KAZINMETR | KZ | Karaganda branch of the RSE "Kazakhstan Institute for metrology" |
| NMC, A*STAR | SG | National Metrology Centre, Agency for Science, Technology and Research, Singapore |

2.2 Measurement standards

Each laboratory taking part in the comparison was requested to produce one standard at the nominal amount fraction of 480 $\mu\text{mol/mol}$ and another at the amount fraction 800 $\mu\text{mol/mol}$. The standards were to be prepared and verified by the participants using their usual procedures. The amount fraction of carbon dioxide was requested to be within $\pm 10 \mu\text{mol/mol}$ of the nominal amount fractions of the cylinders. The carbon dioxide was requested to be produced in a dry air matrix, produced from scrubbed real air or synthetic air that has been blended from pure gases that are the main constituents of air (nitrogen, oxygen, argon) and two other constituents (nitrous oxide and methane). The table below describes the limits of the gas matrix composition of the scrubbed dry real air and synthetic air, which were to be met by participants:

Table 2: Matrix composition limits

| Species | 'Ambient' level mole fraction | Unit | Min amount fraction | Unit | Max amount fraction | Unit |
|------------------|-------------------------------|----------|---------------------|----------|---------------------|----------|
| N ₂ | 0.780876 | mol/mol | 0.7789 | mol/mol | 0.7829 | mol/mol |
| O ₂ | 0.2093335 | mol/mol | 0.2073 | mol/mol | 0.2113 | mol/mol |
| Ar | 0.0093332 | mol/mol | 0.0078 | mol/mol | 0.0108 | mol/mol |
| CH ₄ | 1900 | nmol/mol | 0 | nmol/mol | 1900 | nmol/mol |
| N ₂ O | 330 | nmol/mol | 0 | nmol/mol | 330 | nmol/mol |

Tables 3 and 4 show the reported amount fractions of CO₂ in the mixtures prepared by the participants, expanded uncertainties, pressure and information about cylinders. All participants submitted mixtures with CO₂ amount fraction within 10 $\mu\text{mol mol}^{-1}$ of the nominal values, as requested.

Table 3: Initially submitted values of CO₂ amount fraction, expanded uncertainties, pressure and information about cylinders for 480 $\mu\text{mol/mol}$ level

| Cylinder № | Pressure before measurements, bar | Pressure after measurements, bar | Reported values | | V, L | Cylinder | NMI |
|------------|-----------------------------------|----------------------------------|---|-----------------------------------|------|----------|---------------------|
| | | | CO ₂ amount fraction, $\mu\text{mol mol}^{-1}$ | $U(k=2)$ $\mu\text{mol mol}^{-1}$ | | | |
| D914327 | 95 | 83 | 482.43 | 0.6 | 10 | Luxfer | BelGIM |
| 81205102 | 123 | 116 | 480.27 | 0.45 | 10 | Al cyl. | Ukrmetr-eststandart |
| K772-5 | 80 | 75 | 486.8 | 2.4 | 4 | Al cyl. | KAZINMETR |
| D248767 | 100 | 86 | 479.87 | 0.51 | 5 | Luxfer | NMC, A*STAR |
| M365664 | 90 | 85 | 480.18 | 0.13 | 5 | Luxfer | VNIIM |

Table 4: Initially submitted values of CO₂ amount fractions, expanded uncertainties, pressure and information about cylinders for 800 $\mu\text{mol/mol}$ level

| Cylinder № | Pressure before measurements, bar | Pressure after measurements, bar | Reported values | | V, L | Cylinder | NMI |
|------------|-----------------------------------|----------------------------------|---|-----------------------------------|------|----------|---------------------|
| | | | CO ₂ amount fraction, $\mu\text{mol mol}^{-1}$ | $U(k=2)$ $\mu\text{mol mol}^{-1}$ | | | |
| 5705631 | 94 | 93 | 802.59 | 1.2 | 10 | Luxfer | BelGIM |
| 81205166 | 122 | 121 | 799.99 | 0.83 | 10 | Al cyl. | Ukrmetr-eststandart |
| K772-7 | 90 | 88 | 799.4 | 4 | 4 | Al cyl. | KAZINMETR |
| D248763 | 102 | 101 | 799.37 | 0.76 | 5 | Luxfer | NMC, A*STAR |
| M365707 | 93 | 88 | 800.73 | 0.19 | 5 | Luxfer | VNIIM |

All the participants prepared their standards in accordance with [3] using as a matrix synthetic air that has been blended from pure gases - nitrogen, oxygen, argon, which were within specifications (matrix composition) for all participants as requested in the protocol.

The participants had opportunity to perform stability testing after standards had been returned to them from VNIIM, and before the comparison results were known. This was especially important, since the comparison schedule was significantly disrupted due to the partial closure of NMIs during the pandemic of COVID-19 and delays in the shipment of cylinders.

None of the participants except VNIIM presented isotope ratios of the CO₂ used (it was optional).

A more detailed information on the participants samples, including purity tables and uncertainty

budgets can be found in the participant reports (see Appendix A).

2.3 The schedule

The actual schedule for the project was as follows:

| Date | Action |
|-----------------------------|---|
| June-August 2019 | Preparation of the mixtures by participants |
| February 2020 | Shipment of cylinders to the Pilot (to arrive by 1 of November) |
| | In fact the last cylinder was received in VNIIM in February 2020 |
| August-September 2020 | Analysis of mixtures by VNIIM |
| | Due to pandemic of COVID-19 measurements in VNIIM were carried out in August-September 2020 |
| October 2020 - January 2021 | Return of cylinders to participants |
| February 2021 – June 2021 | 2nd set of analysis of mixtures by participants |
| September 2021 | Distribution of Draft A report |

3 Comparison measurements

3.1 Control mixtures

VNIIM prepared 2 fresh standards at the nominal amount fraction of 480 $\mu\text{mol/mol}$ and 2 standards at 800 $\mu\text{mol/mol}$. The cylinders were verified and one cylinder from each group was used as the reference for COOMET.QM-K120.

In order to provide link to CCQM-K120b and to check trueness these standards were used as reference in the analysis of the appropriate standards, that were prepared for CCQM-K120b. The results confirmed that the difference between the measured (against fresh cylinders) and the assigned value for CCQM-K120b cylinders is within the uncertainty of measurements. The testing was repeated twice in the period of comparison measurements. The results are shown in the Table 5.

Table 5: The results of measurements of the CCQM-K120b standards against new standards

| Cylinder № | Date of preparation, DD.MM.YYYY | Date of measurements, DD.MM.YYYY | Gravimetric value, $\mu\text{mol mol}^{-1}$ | Measured value, $\mu\text{mol mol}^{-1}$ | Difference between the measured and gravimetric values, $\mu\text{mol mol}^{-1}$ | Expanded uncertainty (k=2) of the difference, $\mu\text{mol mol}^{-1}$ |
|------------|---------------------------------|----------------------------------|---|--|--|--|
| M365686 | 10.10.2016 | 09.09.2020 | 480.26 | 480.42 | 0.16 | 0.24 |
| | | 22.09.2020 | | 480.43 | 0.17 | |
| M365711 | 11.10.2016 | 09.09.2020 | 798.9 | 798.50 | -0.40 | 0.43 |
| | | 22.09.2020 | | 798.54 | -0.36 | |

3.2 Instrumentation and measurement procedure

All the measurements at the Pilot laboratory were carried out by Cavity ring-down spectroscopy in August-September 2020.

Instrument: Picarro G2131i + combustion module Picarro

Measurement cell temperature: 45°C

Measurement cell absolute pressure: 18.665 kPa
Data collection: by “Picarro Inc.” software

The 10 cylinders of the comparison were separated into small batches and were analyzed mainly in two cylinders per day with $i=3$ sub-measurements for each.

All cylinders were allowed to equilibrate at laboratory temperature for at least 24 hours. All cylinders were rolled for at least 1 hour to ensure homogeneity of the mixture. The pressure reducer of each cylinder was flushed nine times with the mixture. The cylinder valve was then closed leaving the high pressure side of the pressure reducer at the cylinder pressure and the low pressure side of the pressure reducer at ~ 300 kPa (abs). The cylinders were left stand at least 24 hours, to allow conditioning of the pressure reducers.

The sequence for measurements was as follows:

{nitrogen – analyzed mixture} – [nitrogen – reference standard – nitrogen – analyzed mixture – nitrogen – reference standard – nitrogen] _{$i=3$}

First part of the sequence indicated by braces { } was used for flushing the instrument and preparing for the measurements. The readings of the instrument at this stage were not used in the further calculation.

The measurements of $^{12}\text{CO}_2$ amount fractions were performed at the second part of the sequence indicated by square brackets [].

Subtraction of zero readings (N_2 readings) from the readings of reference and analyzed mixtures is performed in accordance with the following formula

$$A_{sti} = X_{sti} - \left(\frac{N_i + N_{i+1}}{2} \right) \quad (0)$$

where A_{sti} is the corrected reading for i th-input of reference standard,

X_{sti} is the uncorrected reading for i th-input of reference standard,

N_i and N_{i+1} are the uncorrected readings for i th-input and $(i+1)$ th-input of nitrogen appropriately.

Similar formulas are used to obtain $A_{st(i+1)}$ which is the corrected reading for $(i+1)$ th-input of reference standard and A_{ai} which is the corrected reading for i th-input of analyzed mixture.

After subtracting the zero readings (N_2 readings) from the readings of reference and analyzed mixtures according to the formula (0) the following values were obtained: $-[A_{sti} - A_{ai} - A_{st(i+1)}]_{i=3} -$. In the sequence, A_{sti} and A_{ai} are the corrected readings for i th-input of reference standard and analyzed mixture appropriately.

Each reading is the average reading for 5 minutes of every-second measurements.

The instrument was pre-calibrated by reference materials of carbon isotopic composition IAEA-CO-8, IAEA-CH-7 to get $\delta^{13}\text{C}_{\text{VPDB}}$ values. The corresponding readings of the instrument relative to the VPDB are indicated as follows: $-[\delta_{sti} - \delta_{ai} - \delta_{st(i+1)}] -$.

The following formula was used to calculate $^{13}\text{CO}_2$ amount fractions B_{sti} , B_{ai} and $B_{st(i+1)}$

$$B_{sti} = \left(\frac{\delta_{sti}}{1000} + 1 \right) * 0.011118^{(*)} * A_{sti} \quad (1)$$

(*) – according to Werner R.A., Brand W.A. Referencing strategies and techniques in stable isotope ratio analysis. Rapid Commun Mass Spectrom. 2001;15(7):501-519

The measured $\delta^{13}\text{C}_{\text{VPDB}}$ in the mixtures prepared by the participants are shown in the Table 6.

Table 6: The results of measurements of the $\delta^{13}\text{C}_{\text{VPDB}}$ in the mixtures prepared by the participants

| Cylinder № | Measured values | | V, l | Cylinder | NMI |
|------------|---|-------------|------|----------|---------------------|
| | $\delta^{13}\text{C}_{\text{VPDB}}$, ‰ | $U (k=2)$ % | | | |
| D914327 | -47.8 | 0.5 | 10 | Luxfer | BelGIM |
| 81205102 | -43.5 | 0.5 | 10 | Al cyl. | Ukrmetrteststandart |
| K772-5 | -30.4 | 0.5 | 4 | Al cyl. | KAZINMETR |
| D248767 | -28.3 | 0.5 | 5 | Luxfer | NMC, A*STAR |
| D804726 | -51.5 | 0.5 | 5 | Luxfer | VNIIM |
| 5705631 | -47.8 | 0.5 | 10 | Luxfer | BelGIM |
| 81205166 | -43.6 | 0.5 | 10 | Al cyl. | Ukrmetrteststandart |
| K772-7 | -30.3 | 0.5 | 4 | Al cyl. | KAZINMETR |
| D248763 | -28.5 | 0.5 | 5 | Luxfer | NMC. A*STAR |
| D804728 | -51.5 | 0.5 | 5 | Luxfer | VNIIM |

The total amount fraction of CO_2 , taking into account the isotopic composition of the mixture, is calculated in accordance with (2)

$$x_{sti} = A_{sti} + B_{sti} \quad (2)$$

Similar formulas are used to obtain x_{ai} and $x_{st(i+1)}$.

The final amount fraction for the i th-measurement x_i which takes into account drift, is calculated in accordance with (3)

$$x_i = x_{ai} \frac{2 \times G_{st}}{x_{sti} + x_{st(i+1)}} \quad (3)$$

where G_{st} is gravimetric value of CO_2 amount fraction for the reference standard.

Three measurements of x_i were performed each day. Such measurement cycle was repeated for each standard in 3 different days and the average was taken as a result x .

The results of A, B, δ and x for reference materials and participants' samples including their uncertainties are shown in the table 7. $u_{i,meas}$ is the uncertainty of measurements of cylinder i ($\mu\text{mol}/\text{mol}$) ($k=1$).

Table 7. Intermediate measurement results of COOMET.QM-K120

| Cylinder № | Type of cylinder | A, arbitrary units | B, arbitrary units | δ , ‰ | x , $\mu\text{mol mol}^{-1}$ | $u_{i,meas}$, $\mu\text{mol mol}^{-1}$ |
|------------|----------------------|--------------------|--------------------|--------------|--------------------------------|---|
| D914327 | participants' sample | 497.61 | 5.30 | -47.6 | 482.20 | 0.05 |
| 81205102 | participants' sample | 493.63 | 5.28 | -43.3 | 478.39 | 0.05 |
| K772-5 | participants' sample | 502.26 | 5.45 | -30.0 | 486.78 | 0.05 |
| D248767 | participants' sample | 495.38 | 5.38 | -28.0 | 480.19 | 0.05 |
| D804726 | participants' sample | 495.52 | 5.26 | -51.2 | 480.08 | 0.05 |
| 5705631 | participants' sample | 829.04 | 8.82 | -48.2 | 803.14 | 0.14 |
| 81205166 | participants' sample | 823.10 | 8.80 | -44.0 | 797.81 | 0.14 |

| | | | | | | |
|---------|----------------------|--------|------|-------|--------|------|
| | sample | | | | | |
| K772-7 | participants' sample | 825.22 | 8.94 | -30.8 | 799.03 | 0.14 |
| D248763 | participants' sample | 825.16 | 8.96 | -28.9 | 799.33 | 0.14 |
| D804728 | participants' sample | 825.64 | 8.75 | -52.2 | 800.04 | 0.14 |
| D804731 | reference material | 495.41 | 5.25 | -51.2 | - | - |
| D804747 | reference material | 825.62 | 8.75 | -51.9 | - | - |

The uncertainty of measurements $u_{i,meas}$ is calculated according to the following formula

$$u_{i,meas} = \sqrt{(u_x)^2 + (u_\delta)^2} \quad (4)$$

where u_x - standard uncertainty of CO₂ amount fraction, u_δ - standard uncertainty of $\delta^{13}\text{C}_{\text{VPDB}}$.

3.3 Stability measurements by participants

All the participants (except KASINMETR, who assigned to their results substantially larger uncertainties than the other participants) performed stability testing after standards had been returned from VNIIM, and before the comparison results were known. VNIIM (as a participant) and BELGIM confirmed their results, NMC, A*STAR and Ukrmetrteststandart also confirmed the initially presented gravimetric values but provided updated uncertainties.

The results received by NMC, A*STAR and Ukrmetrteststandart before and after measurements at the Pilot laboratory are shown in the table 8.

Table 8 Stability measurements by NMC, A*STAR and Ukrmetrteststandart

| Participant/ Cylinder № | Before measurements at the Pilot lab | | After measurements at the Pilot lab. | | Drift $\mu\text{mol mol}^{-1}$ | Presented lab. values | |
|-------------------------|--------------------------------------|--------------------------------------|--------------------------------------|--------------------------------------|--------------------------------|---------------------------------|--------------------------------------|
| | Value, $\mu\text{mol mol}^{-1}$ | $U (k=2)$, $\mu\text{mol mol}^{-1}$ | Value, $\mu\text{mol mol}^{-1}$ | $U (k=2)$, $\mu\text{mol mol}^{-1}$ | | Value, $\mu\text{mol mol}^{-1}$ | $U (k=2)$, $\mu\text{mol mol}^{-1}$ |
| NMC, A*STAR | | | | | | | |
| D248767 | 480.09 | 0.51 | 480.49 | 0.69 | 0.39 | 479.87 | 0.69 |
| D248763 | 798.94 | 0.76 | 799.34 | 0.90 | 0.40 | 799.37 | 0.90 |
| Ukrmetrteststandart | | | | | | | |
| 81205102 | 480.27 | 0.45 | 481.03 | 0.76 | 0.76 | 480.3 | 0.9 |
| 81205166 | 799.99 | 0.83 | 801.00 | 0.74 | 1.01 | 800.0 | 1.3 |

The detected drift (less than 0,1 % for NMC, A*STAR and less than 0,16 % for Ukrmetrteststandart) and the stability uncertainty contribution are the reason for the participants to update the measurement uncertainty.

3.4 Degrees of equivalence

A unilateral degree of equivalence d_i in key comparisons is defined as

$$d_i = x_{i,lab} - x_{i,KCRV}, \quad (5)$$

and the uncertainty of the difference d_i at 95% level of confidence. Here $x_{i,KCRV}$ denotes the key comparison reference value, and $x_{i,lab}$ the result of laboratory i .

The 40-th meeting of GAWG CCQM [4] recommended not to use the regression analysis of the participants results for assignment of KCRV, but to use direct result of measurements against VNIIM standard.

The standard uncertainty of $x_{i,KCRV}$ can be expressed as

$$u^2(x_{i,KCRV}) = u_{st,prep}^2 + u_{meas}^2 + u_{d(VNIIM/CCQM-K120)}^2 + u_{\Delta}^2 \quad (6)$$

where $u_{st,prep}$ is the standard uncertainty of the VNIIM reference standard, u_{meas} – the standard uncertainty of measurements, $u_{d(VNIIM/CCQM-K120)}$ is the standard uncertainty of VNIIM degree of equivalence in CCQM-K120, u_{Δ} – the standard uncertainty of the difference between the measured (against fresh cylinders) and assigned value for CCQM-K120 cylinders

In this case the standard uncertainty of d_i can be expressed as

$$u^2(d_i) = u_{i,lab}^2 + u_{st,prep}^2 + u_{meas}^2 + u_{d(VNIIM/CCQM-K120)}^2 + u_{\Delta}^2 \quad (7)$$

4 Results

In this section, the results of the key comparison are summarised. In the tables 9 and 10, the following data is presented

$x_{i,lab}$ - result of laboratory i , $\mu\text{mol/mol}$

$u_{i,lab}$ - standard uncertainty of laboratory result¹, $\mu\text{mol/mol}$ ($k=1$)

$x_{i,KCRV}$ - reference value for cylinder of laboratory i , $\mu\text{mol/mol}$

$u_{st,prep}$ - standard uncertainty of the reference standard used in the measurements of $x_{i,lab}$, $\mu\text{mol/mol}$ ($k=1$)

$u_{i,meas}$ - standard uncertainty of measurements of cylinder i , $\mu\text{mol/mol}$ ($k=1$)

$u_{d(VNIIM/CCQM-K120)}$ - standard uncertainty of VNIIM degree of equivalence in CCQM-K120b, $\mu\text{mol/mol}$

u_{Δ} – standard uncertainty of the difference between the measured and assigned values for CCQM-K120b cylinders, $\mu\text{mol/mol}$

d_i - difference between laboratory result and reference value (degree of equivalence), $\mu\text{mol/mol}$

k - assigned coverage factor for degree of equivalence,

$U(d_i)$ - expanded uncertainty of difference d_i , at 95 % level of confidence², $\mu\text{mol/mol}$

The results in graphical form are presented in the figures 1 and 2.

Notes:

¹For obtaining the standard uncertainty of the laboratory results, the expanded uncertainty (stated at a confidence level of 95%) from the laboratory was divided by the reported coverage factor.

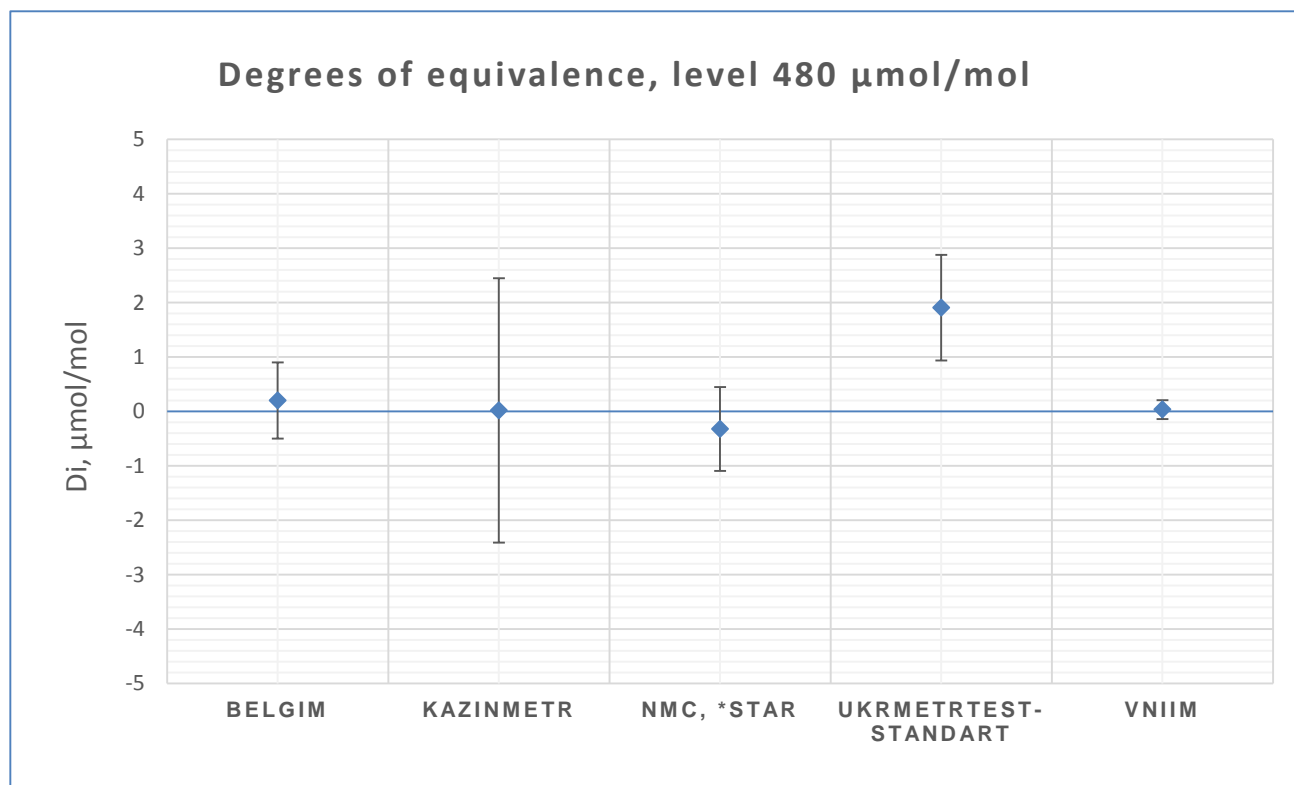
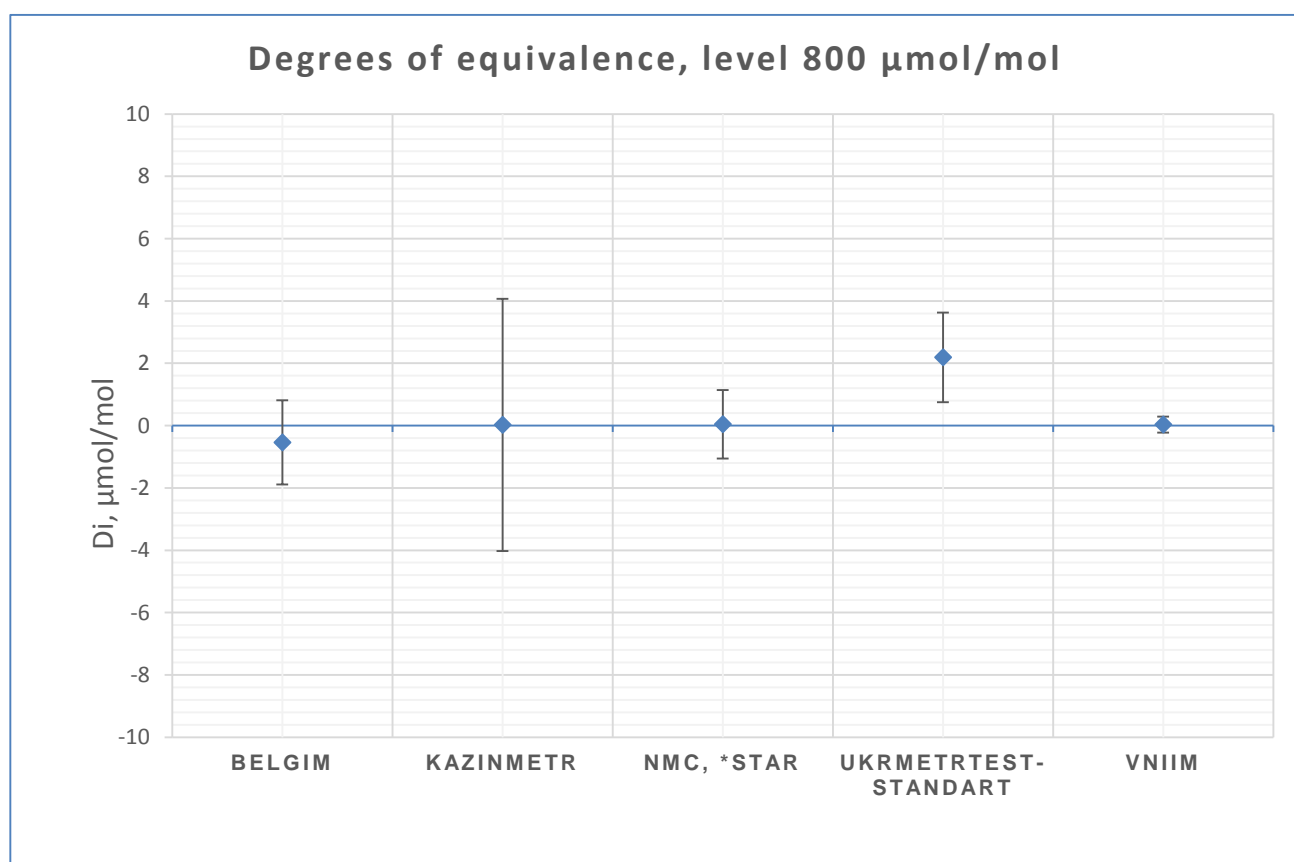
² In the figures 1 and 2 the degrees of equivalence for all participating laboratories are given. The uncertainties are given as 95% confidence intervals as required by the MRA [5]. For the evaluation of uncertainty of the degrees of equivalence, the normal distribution has been assumed, and a coverage factor $k = 2$ was used.

Table 9 : Results of COOMET.QM-K120 – level 480 µmol/mol

| Laboratory | Cylinder | $x_{i,lab}$ | $u_{i,lab}$ | $x_{i,KCRV}$ | $u_{st,prep}$ | $u_{i,meas}$ | $u_{d(VNIIM / CCQM-K120)}$ | u_{Δ} | d_i | k | $U(d_i)$ |
|----------------------|----------|-------------|-------------|--------------|-------------------------|--------------|----------------------------|--------------|-------|-----|----------|
| BelGIM | D914327 | 482.40 | 0.3 | 482.20 | 0.09 | 0.05 | 0.088 | 0.12 | 0.20 | 2 | 0.70 |
| KAZINMETR | K772-5 | 486.80 | 1.2 | 486.78 | 0.09 | 0.05 | 0.088 | 0.12 | 0.02 | 2 | 2.43 |
| NMC, A*STAR | D248767 | 479.87 | 0.34 | 480.19 | 0.09 | 0.05 | 0.088 | 0.12 | -0.32 | 2 | 0.77 |
| Ukrmetrtest-standart | 81205102 | 480.30 | 0.45 | 478.39 | 0.09 | 0.05 | 0.088 | 0.12 | 1.91 | 2 | 0.97 |
| VNIIM | M365664 | 480.18 | 0.065 | 480.145 | 0.059 - $u(x_{i,KCRV})$ | | - | - | 0.035 | 2 | 0.175 |

Table 10: Results of COOMET.QM-K120 – level 800 µmol/mol

| Laboratory | Cylinder | $x_{i,lab}$ | $u_{i,lab}$ | $x_{i,KCRV}$ | $u_{st,prep}$ | $u_{i,meas}$ | $u_{d(VNIIM / CCQM-K120)}$ | u_{Δ} | d_i | k | $U(d_i)$ |
|----------------------|----------|-------------|-------------|--------------|------------------------|--------------|----------------------------|--------------|-------|-----|----------|
| BelGIM | 5705631 | 802.60 | 0.6 | 803.14 | 0.13 | 0.14 | 0.127 | 0.215 | -0.54 | 2 | 1.35 |
| KAZINMETR | K772-7 | 799.40 | 2.0 | 799.38 | 0.13 | 0.14 | 0.127 | 0.215 | 0.02 | 2 | 4.05 |
| NMC, A*STAR | D248763 | 799.37 | 0.45 | 799.33 | 0.13 | 0.14 | 0.127 | 0.215 | 0.04 | 2 | 1.10 |
| Ukrmetrtest-standart | 81205166 | 800.0 | 0.65 | 797.81 | 0.13 | 0.14 | 0.127 | 0.215 | 2.19 | 2 | 1.44 |
| VNIIM | M365707 | 800.730 | 0.095 | 800.697 | 0.084- $u(x_{i,KCRV})$ | | - | - | 0.033 | 2 | 0.253 |

Figure 1 - Degrees of equivalence for level 480 $\mu\text{mol/mol}$ Figure 2 - Degrees of equivalence for level 800 $\mu\text{mol/mol}$

5 Supported CMC claims

The results of this key comparison can be used to support CMCs as described in the final report of CCQM-K120 in the section concerning CCQM-K120.b [1].

CCQM-K120.b comparison tests core skills and competencies required in gravimetric preparation, analytical certification and purity analysis. It is considered as a Track A comparison. It will underpin CO₂ in air and nitrogen claims in a amount fraction range starting at the smallest participant's reported expanded uncertainty and ending at 500 mmol/mol. Participants successful in this comparison may use their result in the flexible scheme and underpin claims for all core mixtures.

6 Discussion and conclusions

The results of this Track A key comparison are satisfactory. All the results except results of one NMI are consistent with the reference values All the results are within ± 0.4 % of the KCRV.

7 References

- [1] Edgar Flores, Joële Viallon et al. CCQM-K120 (Carbon dioxide at background and urban level). Metrologia, V 56, N 1A.
- [2] Brewer P.J., Van der Veen A.M.H., "GAWG strategy for comparisons and CMC claims", CCQM Gas Analysis Working Group, April 2016
- [3] ISO 6142-1:2015. Gas analysis — Preparation of calibration gas mixtures — Part 1: Gravimetric method for Class I mixtures
- [4] Minutes of the 40-meeting of the CCQM GAWG 8-9 APRIL 2019 <https://www.bipm.org/en/committees/cc/ccqm/wg/ccqm-gawg/2019-10-08>
- [5] CIPM, "Mutual recognition of national measurement standards and of calibration and measurement certificates issued by national metrology institutes", Sèvres (F), October 1999

Coordinator

VNIIM, Research department for the State Standards
in the field of physical-chemical measurements
Efremova O.V.
19 Moskovskiy pr., Saint-Petersburg, Russia, 190005
Phone: +7 812 3151145
E-mail fhi@b10.vniim.ru

Completion date: September 2021

Annex A

Reports submitted by participating laboratories

Technical Committee TC 1.8 COOMET
«Physics-chemistry»

Report on results for the Key Comparison
COOMET.QM-K120.b(COOMET project № 772/RU/18)
"Carbon dioxide in air urban level (480-800) $\mu\text{mol/mol}$ "

The general information

| | |
|----------------|--|
| Laboratory: | Belarus, BelGIM, Section for physicochemical and optical measurements, sector for standards and gas mixtures |
| Adress | Minsk, Serova st., 8 |
| Contact person | Mironchik Alexei |
| Phone | +375 17 360 26 37, +375 29 862 11 56 |
| e-mail | spgs@tut.by |

Carbon dioxide mole fraction in standarts for comparison

| No | Cylinder No (date of preparation) | Mole fraction $x_{CO_2.cert}$, $\mu\text{mol/mol}$ | Expandeduncertainty, $U(x_{CO_2.cert})$, $\mu\text{mol/mol}$ | Coverage factor, k |
|----|--------------------------------------|---|---|-------------------------|
| 1 | 5705631 (02.08.2019) | 802,6 | 1,2 | 2 |
| 2 | D914327 (02.08.2019) | 482,4 | 0,6 | 2 |

Matrix compositions for each standard

Standart № 1: cylinder identification number 5705631

| Component | Mole fraction | Unit | Expandeduncertainty | Unit | Coverage factor, k |
|------------------|---------------|----------------------|---------------------|----------------------|-------------------------|
| N ₂ | 0,7789302 | mol/mol | 0,0000084 | mol/mol | 2 |
| O ₂ | 0,2109324 | mol/mol | 0,0000082 | mol/mol | 2 |
| Ar | 0,0093335 | mol/mol | 0,0000024 | mol/mol | 2 |
| CH ₄ | 15,1 | $\eta\text{mol/mol}$ | 13,4 | $\eta\text{mol/mol}$ | 2 |
| H ₂ O | 1070 | $\eta\text{mol/mol}$ | 1040 | $\eta\text{mol/mol}$ | 2 |
| CO | 88,9 | $\eta\text{mol/mol}$ | 90 | $\eta\text{mol/mol}$ | 2 |
| H ₂ | 4,1 | $\eta\text{mol/mol}$ | 4,4 | $\eta\text{mol/mol}$ | 2 |

Standart № 2: cylinder identification number D914327

| Component | Mole fraction | Unit | Expanded uncertainty | Unit | Coverage factor, k |
|------------------|---------------|----------|----------------------|----------|----------------------|
| N ₂ | 0,7803529 | mol/mol | 0,0000082 | mol/mol | 2 |
| O ₂ | 0,2097935 | mol/mol | 0,0000080 | mol/mol | 2 |
| Ar | 0,0093700 | mol/mol | 0,0000024 | mol/mol | 2 |
| CH ₄ | 14,9 | ηmol/mol | 13,4 | ηmol/mol | 2 |
| H ₂ O | 1070 | ηmol/mol | 1060 | ηmol/mol | 2 |
| CO | 88,9 | ηmol/mol | 92 | ηmol/mol | 2 |
| H ₂ | 4,1 | ηmol/mol | 4,6 | ηmol/mol | 2 |

Purity tables with uncertainties for the nominally pure parent gases

Purity table with uncertainties for the nominally pure CO₂ parent gas

For a standarts preparation was used nominally pure CO₂(purity extent 5.3).Composition provided by the supplier certificate and composition taken over to calculation in accordance ISO/DIS 19229 are resulted in tables below.

Composition provided by the supplier certificate

| Component | Value | Unit |
|------------------|-----------|----------------------------|
| CO ₂ | ≥ 99,9993 | mol/mol · 10 ⁻² |
| O ₂ | ≤ 0,0002 | mol/mol · 10 ⁻² |
| N ₂ | ≤ 0,0003 | mol/mol · 10 ⁻² |
| CH ₄ | ≤ 0,0001 | mol/mol · 10 ⁻² |
| CO | ≤ 0,00005 | mol/mol · 10 ⁻² |
| H ₂ O | ≤ 0,0001 | mol/mol · 10 ⁻² |

Composition taken over to calculation in accordance ISO/DIS 19229

| Component | Mole fraction | Unit | Standart uncertainty | Unit |
|------------------|---------------|----------|----------------------|----------|
| CO ₂ | 0,99999625 | mol/mol | 0,00000117 | mol/mol |
| O ₂ | 1000 | ηmol/mol | 600 | ηmol/mol |
| N ₂ | 1500 | ηmol/mol | 900 | ηmol/mol |
| CH ₄ | 500 | ηmol/mol | 300 | ηmol/mol |
| CO | 250 | ηmol/mol | 140 | ηmol/mol |
| H ₂ O | 500 | ηmol/mol | 300 | ηmol/mol |

Purity table with uncertainties for the nominally pure O₂ parent gas

For a standards preparation was used nominally pure HiQ O₂ (purity extent 6.0). Composition provided by the supplier certificate and composition taken over to calculation in accordance ISO/DIS 19229 are resulted in tables below.

Composition provided by the supplier certificate

| Component | Value | Unit |
|------------------|-----------|----------------------------|
| O ₂ | ≥ 99,9999 | mol/mol · 10 ⁻² |
| N ₂ | ≤ 0,00005 | mol/mol · 10 ⁻² |
| CO ₂ | ≤ 0,00001 | mol/mol · 10 ⁻² |
| CH ₄ | ≤ 0,00001 | mol/mol · 10 ⁻² |
| CO | ≤ 0,00001 | mol/mol · 10 ⁻² |
| H ₂ O | ≤ 0,00005 | mol/mol · 10 ⁻² |
| Ar | ≤ 0,0001 | mol/mol · 10 ⁻² |

Composition taken over to calculation in accordance ISO/DIS 19229

| Component | Mole fraction | Unit | Standart uncertainty | Unit |
|------------------|---------------|----------|----------------------|----------|
| O ₂ | 0,99999885 | mol/mol | 0,00000036 | mol/mol |
| N ₂ | 250 | ηmol/mol | 140 | ηmol/mol |
| CO ₂ | 50 | ηmol/mol | 30 | ηmol/mol |
| CH ₄ | 50 | ηmol/mol | 30 | ηmol/mol |
| CO | 50 | ηmol/mol | 30 | ηmol/mol |
| H ₂ O | 250 | ηmol/mol | 140 | ηmol/mol |
| Ar | 500 | ηmol/mol | 300 | ηmol/mol |

Purity table with uncertainties for the nominally pure N₂ parent gas

For a standards preparation was used nominally pure N₂ (purity extent 6.0). Composition provided by the supplier certificate and composition taken over to calculation in accordance ISO/DIS 19229 are resulted in tables below.

Composition provided by the supplier certificate

| Component | Value | Unit |
|------------------|------------|----------------------------|
| N ₂ | ≥ 99,9999 | mol/mol · 10 ⁻² |
| O ₂ | ≤ 0,000055 | mol/mol · 10 ⁻² |
| CO ₂ | ≤ 0,00002 | mol/mol · 10 ⁻² |
| CH ₄ | ≤ 0,000001 | mol/mol · 10 ⁻² |
| CO | ≤ 0,00002 | mol/mol · 10 ⁻² |
| H ₂ O | ≤ 0,00025 | mol/mol · 10 ⁻² |
| H ₂ | ≤ 0,000001 | mol/mol · 10 ⁻² |

Composition taken over to calculation in accordance ISO/DIS 19229

| Component | Mole fraction | Unit | Standart uncertainty | Unit |
|------------------|---------------|----------|----------------------|----------|
| N ₂ | 0,99999821 | mol/mol | 0,00000072 | mol/mol |
| O ₂ | 280 | ηmol/mol | 160 | ηmol/mol |
| CO ₂ | 100 | ηmol/mol | 60 | ηmol/mol |
| CH ₄ | 5 | ηmol/mol | 3 | ηmol/mol |
| CO | 100 | ηmol/mol | 60 | ηmol/mol |
| H ₂ O | 1300 | ηmol/mol | 700 | ηmol/mol |
| H ₂ | 5 | ηmol/mol | 3 | ηmol/mol |

Purity table with uncertainties for the nominally pure Ar parent gas

For a standards preparation was used nominally pure Ar(purity extent 6.0).Composition provided by the supplier certificate and composition taken over to calculation in accordance ISO/DIS 19229 are resulted in tables below

Composition provided by the supplier certificate

| Component | Value | Unit |
|------------------|------------|----------------------------|
| Ar | ≥ 99,9999 | mol/mol · 10 ⁻² |
| N ₂ | ≤ 0,000045 | mol/mol · 10 ⁻² |
| O ₂ | ≤ 0,00003 | mol/mol · 10 ⁻² |
| CO ₂ | ≤ 0,00001 | mol/mol · 10 ⁻² |
| CH ₄ | ≤ 0,000005 | mol/mol · 10 ⁻² |
| CO | ≤ 0,000005 | mol/mol · 10 ⁻² |
| H ₂ O | ≤ 0,00005 | mol/mol · 10 ⁻² |
| H ₂ | ≤ 0,000005 | mol/mol · 10 ⁻² |

Composition taken over to calculation in accordance ISO/DIS 19229

| Component | Mole fraction | Unit | Standart uncertainty | Unit |
|------------------|---------------|----------|----------------------|----------|
| Ar | 0,999999245 | mol/mol | 0,000000215 | mol/mol |
| N ₂ | 230 | ηmol/mol | 130 | ηmol/mol |
| O ₂ | 150 | ηmol/mol | 90 | ηmol/mol |
| CO ₂ | 50 | ηmol/mol | 30 | ηmol/mol |
| CH ₄ | 25 | ηmol/mol | 14 | ηmol/mol |
| CO | 25 | ηmol/mol | 14 | ηmol/mol |
| H ₂ O | 250 | ηmol/mol | 140 | ηmol/mol |
| H ₂ | 25 | ηmol/mol | 14 | ηmol/mol |

A brief outline of the dilution series undertaken to produce the final mixtures

Final mixtures are obtained by using 2-time dilution: 100 % → 2 % → final mixtures.

Intermediate mixture was determined by a gravimetric method according to ISO 6142. Molar masses of components and their associated uncertainties are derived from ISO 14912:2003 (E). Intermediate mixture composition resulted in table below.

Intermediate mixture composition 2 % CO₂-N₂

| Component | Mole fraction | Unit | Standart uncertainty | Unit |
|-----------|---------------|------|----------------------|------|
|-----------|---------------|------|----------------------|------|

| | | | | |
|------------------|--------------|----------|------------|----------|
| N ₂ | 0,9791762818 | mol/mol | 0,00030852 | mol/mol |
| CO ₂ | 0,020822 | mol/mol | 0,000003 | mol/mol |
| O ₂ | 295 | ηmol/mol | 157 | ηmol/mol |
| CO | 103 | ηmol/mol | 59 | ηmol/mol |
| CH ₄ | 15,3 | ηmol/mol | 6,9 | ηmol/mol |
| H ₂ O | 1300 | ηmol/mol | 700 | ηmol/mol |
| H ₂ | 4,9 | ηmol/mol | 2,94 | ηmol/mol |

Verification procedure applied to the final mixtures

Verification of composition was performed on a gas chromatographer (GC) "Crystal 5000" fitted with TCD in accordance with ISO 6142, ISO 6143. Gas-carrier is helium.

Verification was made to two stages with use of four CO₂-Air gas mixtures, one of which was the standard for comparison, within the linear range of an analytical method.

Gas mixture compositions used for verification

| No | Cylinder identification number | CO ₂ mole fraction, μmol/mol | Standard uncertainty, according to gravimetric calculation, μmol/mol |
|----|--------------------------------|---|--|
| 1 | 5145 | 851,30 | 0,16 |
| 2 | 5335 | 452,11 | 0,14 |
| 3 | 5142 | 652,02 | 0,17 |
| 4 | D914327 | 482,43 | 0,09 |
| 5 | 5705631 | 802,59 | 0,13 |

Measure of verification is requirement performance:

$$|X_{CO_2} - X_{CO_2,ver}| \leq 2 \sqrt{u^2(X_{CO_2,prep}) + u^2(X_{CO_2,ver})}, \quad (1)$$

$X_{CO_2,ver}$ и $u(X_{CO_2,ver})$ - measured value of molar fraction CO₂ in the standard for comparison and standard uncertainty of measuring accordingly, counted according to ISO 6143;

$u(X_{CO_2,prep})$ - standard uncertainty of gravimetric preparation taking into account uncertainty of the instability, evaluated by formula

$$u(X_{CO_2,prep}) = \sqrt{u^2(X_{CO_2}) + u^2(X_{CO_2,stab})}, \quad (2)$$

где $u(X_{CO_2})$ - standard uncertainty of gravimetric preparation;

$u(X_{CO_2,stab})$ - standard uncertainty of the instability, evaluated during stability researches for such type mixtures; $u(X_{CO_2,stab}) = 0,1\%$ rel.

Total standard uncertainty of molar fraction CO₂ evaluated by following formula:

$$u_c(X_{CO_2}) = \frac{1}{2} \sqrt{u^2(X_{CO_2,prep}) + u^2(X_{CO_2,ver}) + (X_{CO_2} - X_{CO_2,ver})^2}. \quad (3)$$

Results of verification (date of verification – 11.08.2019)

| Cylinder identification number | X_{CO_2} , μmol/mol | $u^2(X_{CO_2})$, μmol/mol | $X_{CO_2,ver}$, μmol/mol | $u(X_{CO_2,ver})$, μmol/mol | $ X_{CO_2} - X_{CO_2,ver} $, μmol/mol | $u_c(X_{CO_2})$, μmol/mol |
|--------------------------------|-----------------------|----------------------------|---------------------------|------------------------------|--|----------------------------|
| | | | | | | |

| | | | | | | |
|---------|--------|------|--------|------|------|------|
| D914327 | 482,43 | 0,09 | 482,37 | 0,26 | 0,06 | 0,28 |
| 5705631 | 802,59 | 0,13 | 801,88 | 0,32 | 0,71 | 0,56 |

Cylinder pressure before shipment to VNIIM – 9,9 MPa.

Checking the stability of the CO₂ content in the comparison samples

Upon returning the cylinders from the coordinator, the stability of the composition of the samples was checked. The stability checking was performed on a gas chromatographer (GC) "Crystal 5000" fitted with TCD in accordance with ISO 6143 using 5 samples, two of which are samples for comparisons, within the linear range of the analytical method.

The criterion for confirming the stability of the composition is the fulfillment of condition (1) were $u(X_{CO_2,prep})$ - standard uncertainty of gravimetric preparation.

Date of checking stability – 18.02.2021.

The test results are listed in the table below.

| Cylinder identification number | $X_{CO_2,prep}$, μmol/mol | $u(X_{CO_2,prep})$, μmol/mol | $X_{CO_2,ver}$, μmol/mol | $u(X_{CO_2,ver})$, μmol/mol | $ X_{CO_2,prep} - X_{CO_2,ver} $ μmol/mol | $2\sqrt{u^2(X_{CO_2,prep}) + u^2(X_{CO_2,ver})}$ μmol/mol |
|--------------------------------|-------------------------------|----------------------------------|------------------------------|---------------------------------|--|--|
| 5335 | 453,55 | 0,17 | 453,8 | 0,4 | 0,33 | 0,82 |
| D914327 | 482,43 | 0,09 | 482,1 | 0,4 | 0,11 | 0,72 |
| 5142 | 651,23 | 0,22 | 651,12 | 0,28 | 0,51 | 0,66 |
| 5705631 | 802,59 | 0,13 | 803,1 | 0,3 | 0,58 | 0,76 |
| 5145 | 855,30 | 0,25 | 854,72 | 0,28 | 0,33 | 0,82 |

Conclusion

The declared gravimetric value of the mole fraction of CO₂ is confirmed within the declared uncertainty.

Report COOMET.QM-K120

General information

| | |
|----------------|--|
| Institute | Karaganda branch of the RSE "Kazakhstan Institute metrology" |
| Address | Karaganda, st. Anzherskaya, 22/2 |
| Contact person | Alexandrov Vladimir Vladimirovich |
| Phone | 8 (7212) 44-09-25 |
| E-mail | Alexandrov@kazinmetr.kz |

Values provided by NMI. Carbon dioxide content.

| № | Cylinder identification number | Molar fraction of carbon dioxide, $X_{CO_2, cert}$ $\mu\text{mol} / \text{mol}$ | Expanded uncertainty $U(X_{CO_2, cert})$ $\mu\text{mol} / \text{mol}$ | Coverage ratio |
|---|--------------------------------|---|---|----------------|
| 1 | K772-5 | 486,8 | 2,4 | 2 |
| 2 | K772-7 | 799,4 | 4,0 | 2 |

Values provided by NMI. Matrix composition.

Cylinder No. K772-5

| Component | Molar fraction | Unit of measurement | Expanded uncertainty | Coverage ratio |
|------------------|----------------|------------------------------|----------------------|----------------|
| N ₂ | 0,780935 | mol/mol | 0,004 | 2 |
| O ₂ | 0,209214 | mol/mol | 0,001 | 2 |
| Ar | 0,009362 | mol/mol | 0,00009 | 2 |
| CH ₄ | 1,4 | $\mu\text{mol} / \text{mol}$ | 0,3 | 2 |
| N ₂ O | - | - | - | - |

Cylinder No. K772-7

| Component | Molar fraction | Unit of measurement | Expanded uncertainty | Coverage ratio |
|------------------|----------------|------------------------------|----------------------|----------------|
| N ₂ | 0,780402 | mol/mol | 0,004 | 2 |
| O ₂ | 0,209405 | mol/mol | 0,001 | 2 |
| Ar | 0,009392 | mol/mol | 0,00009 | 2 |
| CH ₄ | 1,4 | $\mu\text{mol} / \text{mol}$ | 0,3 | 2 |
| N ₂ O | - | - | - | - |

Additional Information

Purity table for nominally pure CO₂ feed gas

| Impurity | Method of measurement | Molar fraction, $\mu\text{mol} / \text{mol}$ | Standard uncertainty of molar fraction, $\mu\text{mol} / \text{mol}$ |
|-----------------|------------------------------|--|--|
| N ₂ | GC-TCD | 24,2 | 4,8 |
| CO | GC-FID | 1,0 | 0,3 |
| O ₂ | GC –thermo-chemical detector | 6,0 | 1,0 |
| H ₂ | GC –thermo-chemical detector | 0,5 | 0,2 |
| CH ₄ | GC-FID | 0,3 | 0,1 |
| CO ₂ | Calculation | 999 968 | 5,0 |

Purity table for nominally pure N₂ feed gas

| Impurity | Method of measurement | Molar fraction, $\mu\text{mol} / \text{mol}$ | Standard uncertainty of molar fraction, $\mu\text{mol} / \text{mol}$ |
|-----------------|------------------------------|--|--|
| O ₂ | GC –thermo-chemical detector | 10,1 | 3,0 |
| H ₂ | GC –thermo-chemical detector | 0,2 | 0,1 |
| CH ₄ | GC-FID | 0,2 | 0,1 |
| CO | GC-FID | 0,3 | 0,1 |
| CO ₂ | GC-FID | 0,2 | 0,1 |
| N ₂ | Calculation | 999 989 | 3,0 |

Purity table for nominally pure O₂ feed gas

| Impurity | Method of measurement | Molar fraction, $\mu\text{mol} / \text{mol}$ | Standard uncertainty of molar fraction, $\mu\text{mol} / \text{mol}$ |
|-----------------|-----------------------|--|--|
| N ₂ | GC-TCD | 367 | 37,0 |
| CH ₄ | GC-FID | 6,1 | 0,6 |
| CO ₂ | GC-FID | 2,0 | 0,4 |
| O ₂ | Calculation | 999 625 | 37,0 |

Purity table for nominally pure Ar feed gas

| Impurity | Method of measurement | Molar fraction, $\mu\text{mol} / \text{mol}$ | Standard uncertainty of molar fraction, $\mu\text{mol} / \text{mol}$ |
|-----------------|-----------------------|--|--|
| CO ₂ | GC-FID | 0,2 | 0,1 |
| N ₂ | GC-TCD | 15,0 | 7,5 |

| | | | |
|-----------------|------------------------------|---------|-----|
| O ₂ | GC –thermo-chemical detector | 3,5 | 1,7 |
| H ₂ | GC –thermo-chemical detector | 0,7 | 0,4 |
| CH ₄ | GC-FID | 0,2 | 0,1 |
| CO | GC-FID | 1,1 | 0,4 |
| Ar | Calculation | 999 979 | 7,7 |

The following series of dilutions were used to prepare the target mixtures:

- K772-1(CO₂-Ar) >K772-3 (CO₂-Ar-N₂) >K772-5 (CO₂-Ar-O₂-N₂)andK772-8 (CO₂-Ar-O₂-N₂) (for verification)

- K772-2 (CO₂-Ar) >K772-4 (CO₂-Ar-N₂) >K772-7 (CO₂-Ar-O₂-N₂)andK772-6 (CO₂-Ar-O₂-N₂) (for verification)

The nominal values of the molar fraction of components in intermediate gas mixtures are presented in tables 1 and 2.

Table 1

| Cylinder No. | Molar fraction, mol/mol | |
|--------------|-------------------------|-------|
| | CO ₂ | Ar |
| K772-1 | 0,049 | 0,951 |
| K772-2 | 0,078 | 0,922 |

Table 2

| Cylinder No. | Molar fraction, mol/mol | | |
|--------------|-------------------------|-------|----------------|
| | CO ₂ | Ar | N ₂ |
| K772-3 | 0,006 | 0,112 | 0,882 |
| K772-4 | 0,012 | 0,134 | 0,854 |

The pressure in the cylinders before being sent to the coordinating laboratory was 10.0 MPa.

Report form COOMET.QM-K120 (1)

(submitted 12/02/2020)

A1. General information

| | |
|----------------|--|
| Institute | National Metrology Centre (NMC), Agency for Science, Technology and Research (A*STAR), Singapore |
| Address | 1 Science Park Drive, Singapore 118221 |
| Contact person | Kai Fuu Ming |
| Telephone | +65 6279 1942 |
| Email* | Kai_fuu_ming@nmc.a-star.edu.sg |

A2. NMI submitted values. Carbon dioxide mole fraction

| | Cylinder Identification number | Carbon dioxide mole fraction $x_{\text{CO}_2, \text{cert}}$ $\mu\text{mol/mol}$ | Expanded uncertainty $U(x_{\text{CO}_2, \text{cert}})$ $\mu\text{mol/mol}$ | Coverage factor |
|---|--------------------------------|---|--|-----------------|
| 1 | D248767 | 479.87 | 0.51 | 2 |
| 2 | D248763 | 799.37 | 0.76 | 2 |

A3. NMI submitted values

Matrix compositions (for each standard submitted):

(Standard 1) Cylinder Identification Number: D248767

| Component | Mole fraction Value | Unit | Expanded Uncertainty | Unit | Coverage Factor |
|-----------------|---------------------|---------------------|----------------------|---------------------|-----------------|
| N ₂ | 0.780894 | mol/mol | 0.000016 | mol/mol | 2 |
| O ₂ | 0.209233 | mol/mol | 0.000015 | mol/mol | 2 |
| Ar | 0.009393 | mol/mol | 0.000003 | mol/mol | 2 |
| CH ₄ | 0.050 | $\mu\text{mol/mol}$ | 0.044 | $\mu\text{mol/mol}$ | 2 |

(Standard2)CylinderIdentificationNumber: D248763

| Component | Mole fraction Value | Unit | Expanded Uncertainty | Unit | Coverage Factor |
|-----------------|---------------------|----------|----------------------|----------|-----------------|
| N ₂ | 0.780338 | mol/mol | 0.000016 | mol/mol | 2 |
| O ₂ | 0.209459 | mol/mol | 0.000015 | mol/mol | 2 |
| Ar | 0.009403 | mol/mol | 0.000003 | mol/mol | 2 |
| CH ₄ | 0.050 | μmol/mol | 0.042 | μmol/mol | 2 |

A4. Uncertainty Budget

Uncertainty budgets for the CO₂ mole fraction values reported

| Cylinder Identification Number | Gravimetric preparation uncertainty, μmol/mol | Verification uncertainty, μmol/mol | Combined uncertainty, μmol/mol | Expanded uncertainty, μmol/mol | Coverage factor |
|--------------------------------|---|------------------------------------|--------------------------------|--------------------------------|-----------------|
| D248767 | 0.11 | 0.23 | 0.26 | 0.51 | k=2 |
| D248763 | 0.13 | 0.36 | 0.38 | 0.76 | k=2 |

5. Additional information

Purity table for Pure CO₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|-------------------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 2.000E-07 | Normal | 3.325E-09 |
| Impurity | O ₂ | 6.000E-08 | Normal | 3.139E-09 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | C ₂ H ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 2.500E-06 | Rectangular | 1.443E-06 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ | 1.200E-07 | Normal | 6.928E-08 |
| Impurity | Ar | 9.000E-08 | Normal | 6.213E-09 |
| Balance gas | CO ₂ | 0.99999691 | | 1.446E-06 |

Purity table for Pure N₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|------------|----------------|-------------------------|--------------|--------------------------------|
| Impurity | O ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ | 2.500E-08 | Rectangular | 1.443E-08 |

| | | | | |
|-------------|------------------|------------|-------------|-----------|
| Impurity | CO ₂ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 1.000E-08 | Rectangular | 5.774E-09 |
| Balance gas | N ₂ | 0.99999982 | | 4.822E-08 |

Purity table for pure O₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 5.000E-07 | Rectangular | 2.887E-07 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 2.500E-07 | Rectangular | 1.443E-07 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | Ar | 5.000E-08 | Rectangular | 2.887E-08 |
| Balance gas | O ₂ | 0.99999905 | | 3.272E-07 |

Purity table for pure Ar

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 1.000E-06 | Rectangular | 5.774E-07 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ O | 5.000E-07 | Rectangular | 2.887E-07 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | O ₂ | 5.000E-07 | Rectangular | 2.887E-07 |
| Balance gas | Ar | 0.99999790 | | 7.080E-07 |

Gas mixture verification

The carbon dioxide in air mixtures were analyzed on a cavity ring-down spectroscopy (CRDS) instrument, i.e., Picarro G2401 Analyzer. Verification of the mixtures was carried out using our freshly prepared standards. Cylinders were equipped with pressure reducers and they were flushed three times before measurement. Cylinders were then connected to a mass flow controller (MFC) and the flow rate was fixed at 500 sccm. In the sample line between MFC and CRDS, there was a bypass to allow excessive gas to be vented out. Each cylinder was measured and data recorded for 15 minutes. The readings from 13 to 14 minutes were selected for the determination of average values for each cylinder at each measurement.

Measurements of all gas mixtures have been repeated for 3 days. The deviation between the measured value

and gravimetric value for the prepared gas mixtures are below the verification uncertainty.

Total uncertainty estimation

The uncertainties of the gas mixture has been estimated by combining the gravimetric preparation uncertainty and the verification uncertainty. The gravimetric preparation uncertainty includes contribution from impurity of source gas (CO₂, Ar, O₂, N₂) and premix, molar mass and cylinder weighing process. The verification uncertainty includes contribution from the day-to-day variation, measurement repeatability, consistency check error and regression analysis residual error.

Uncertainty budgets for the CO₂ mole fraction values reported

| Cylinder Identification Number | Gravimetric preparation uncertainty, $\mu\text{mol/mol}$ | Verification uncertainty, $\mu\text{mol/mol}$ | Combined uncertainty, $\mu\text{mol/mol}$ | Expanded uncertainty, $\mu\text{mol/mol}$ | Coverage factor |
|--------------------------------|--|---|---|---|-----------------|
| D248767 | 0.11 | 0.23 | 0.26 | 0.51 | k=2 |
| D248763 | 0.13 | 0.36 | 0.38 | 0.76 | k=2 |

Report form COOMET.QM-K120 (2)

(submitted 28/07/2021)

A1. General information

| | |
|----------------|--|
| Institute | National Metrology Centre (NMC), Agency for Science, Technology and Research (A*STAR), Singapore |
| Address | 1 Science Park Drive, Singapore 118221 |
| Contact person | Kai Fuu Ming |
| Telephone | +65 6279 1942 |
| Email* | Kai_fuu_ming@nmc.a-star.edu.sg |

A2. NMI submitted values. Carbon dioxide mole fraction

| | Cylinder Identification number | Carbon dioxide mole fraction $X_{CO_2, cert}$ $\mu\text{mol/mol}$ | Expanded uncertainty $U(x_{CO_2, cert})$ $\mu\text{mol/mol}$ | Coverage factor |
|---|--------------------------------|---|--|-----------------|
| 1 | D248767 | 479.87 | 0.69 | 2 |
| 2 | D248763 | 799.37 | 0.90 | 2 |

A3. NMI submitted values

Matrix compositions (for each standard submitted):

(Standard 1) Cylinder Identification Number: D248767

| Component | Mole fraction Value | Unit | Expanded Uncertainty | Unit | Coverage Factor |
|-----------------|---------------------|---------------------|----------------------|---------------------|-----------------|
| N ₂ | 0.780894 | mol/mol | 0.000016 | mol/mol | 2 |
| O ₂ | 0.209233 | mol/mol | 0.000015 | mol/mol | 2 |
| Ar | 0.009393 | mol/mol | 0.000003 | mol/mol | 2 |
| CH ₄ | 0.050 | $\mu\text{mol/mol}$ | 0.044 | $\mu\text{mol/mol}$ | 2 |

(Standard2)CylinderIdentificationNumber: D248763

| Component | Mole fraction Value | Unit | Expanded Uncertainty | Unit | Coverage Factor |
|-----------------|---------------------|----------|----------------------|----------|-----------------|
| N ₂ | 0.780338 | mol/mol | 0.000016 | mol/mol | 2 |
| O ₂ | 0.209459 | mol/mol | 0.000015 | mol/mol | 2 |
| Ar | 0.009403 | mol/mol | 0.000003 | mol/mol | 2 |
| CH ₄ | 0.050 | μmol/mol | 0.042 | μmol/mol | 2 |

A4. Uncertainty Budget

Uncertainty budgets for the reported CO₂ mole fraction values

| Cylinder Identification Number | Gravimetric preparation uncertainty, μmol/mol | Verification uncertainty, μmol/mol | Stability uncertainty, μmol/mol | Combined uncertainty, μmol/mol | Expanded uncertainty, μmol/mol | Coverage factor |
|--------------------------------|---|------------------------------------|---------------------------------|--------------------------------|--------------------------------|-----------------|
| D248767 | 0.11 | 0.23 | 0.23 | 0.34 | 0.69 | k=2 |
| D248763 | 0.13 | 0.36 | 0.23 | 0.45 | 0.90 | k=2 |

A5. Additional information

Purity table for Pure CO₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|-------------------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 2.000E-07 | Normal | 3.325E-09 |
| Impurity | O ₂ | 6.000E-08 | Normal | 3.139E-09 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | C ₂ H ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 2.500E-06 | Rectangular | 1.443E-06 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ | 1.200E-07 | Normal | 6.928E-08 |
| Impurity | Ar | 9.000E-08 | Normal | 6.213E-09 |
| Balance gas | CO ₂ | 0.99999691 | | 1.446E-06 |

Purity table for Pure N₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|------------|----------------|-------------------------|--------------|--------------------------------|
| Impurity | O ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |

| | | | | |
|-------------|------------------|------------|-------------|-----------|
| Impurity | H ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO ₂ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 1.000E-08 | Rectangular | 5.774E-09 |
| Balance gas | N ₂ | 0.99999982 | | 4.822E-08 |

Purity table for pure O₂

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 5.000E-07 | Rectangular | 2.887E-07 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | H ₂ O | 2.500E-07 | Rectangular | 1.443E-07 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | Ar | 5.000E-08 | Rectangular | 2.887E-08 |
| Balance gas | O ₂ | 0.99999905 | | 3.272E-07 |

Purity table for pure Ar

| Components | | Concentration (mol/mol) | Distribution | Standard Uncertainty (mol/mol) |
|-------------|------------------|-------------------------|--------------|--------------------------------|
| Impurity | N ₂ | 1.000E-06 | Rectangular | 5.774E-07 |
| Impurity | CO | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | CO ₂ | 2.500E-08 | Rectangular | 1.443E-08 |
| Impurity | H ₂ O | 5.000E-07 | Rectangular | 2.887E-07 |
| Impurity | CH ₄ | 5.000E-08 | Rectangular | 2.887E-08 |
| Impurity | O ₂ | 5.000E-07 | Rectangular | 2.887E-07 |
| Balance gas | Ar | 0.99999790 | | 7.080E-07 |

Gas mixture verification

The carbon dioxide in air mixtures were analyzed on a cavity ring-down spectroscopy (CRDS) instrument, i.e., Picarro G2401 Analyzer. Verification of the mixtures was carried out using our freshly prepared standards. Cylinders were equipped with pressure reducers and they were flushed three times before measurement. Cylinders were then connected to a mass flow controller (MFC) and the flow rate was fixed at 500 sccm. In the sample line between MFC and CRDS, there was a bypass to allow excessive gas to be vented out. Each cylinder was measured and data recorded for 15 minutes. The readings from 13 to 14 minutes were selected for the determination of average values for each cylinder at each measurement.

Measurements of all gas mixtures have been repeated for 3 days. The deviation between the measured value and gravimetric value for the prepared gas mixtures are below the verification uncertainty.

Gas mixture stability check

The carbon dioxide in air mixtures (D248767, D248763) were returned to NMC and analyzed again in Mar 2021 using a CRDS instrument, i.e., Picarro G2401 Analyzer. Cylinders were equipped with pressure reducers and they were flushed three times before measurement. Cylinders were then connected to a MFC and the flow rate was fixed at 500 sccm. The analyser's readings of 1 minute were used for the determination of average concentration values for each cylinder. Measurements for the two cylinders have been repeated in 2 days.

The deviation between the measured value in Jul 2019 and Mar 2021 (Δx) are shown in the table below. The standard uncertainty due to stability ($k=1$) was derived as $u_s = \Delta x / \sqrt{3}$.

Stability check for the two gas mixtures (D248767, D248763)

| Cylinder Identification Number | GSM mixture std | measured value in Jul 2019, ppm | measured value in Mar 2021, ppm | Deviation between two measurements (Δx), ppm | uncertainty due to stability ($k=1$), ppm |
|--------------------------------|-----------------|---------------------------------|---------------------------------|--|---|
| D248767 | PSM118767 | 480.09 | 480.49 | 0.39 | 0.23 |
| D248763 | PSM118763 | 798.94 | 799.34 | 0.40 | 0.23 |

Total uncertainty estimation

The uncertainties of the gas mixture has been estimated by combining the gravimetric preparation uncertainty, the verification uncertainty and the stability uncertainty. The gravimetric preparation uncertainty includes contribution from impurity of source gas (CO_2 , Ar, O_2 , N_2) and premix, molar mass and cylinder weighing process. The verification uncertainty includes contribution from the day-to-day variation, measurement repeatability, consistency check error and regression analysis residual error.

Uncertainty budgets for the reported CO_2 mole fraction values

| Cylinder Identification Number | Gravimetric preparation uncertainty, $\mu\text{mol/mol}$ | Verification uncertainty, $\mu\text{mol/mol}$ | Stability uncertainty, $\mu\text{mol/mol}$ | Combined uncertainty, $\mu\text{mol/mol}$ | Expanded uncertainty, $\mu\text{mol/mol}$ | Coverage factor |
|--------------------------------|--|---|--|---|---|-----------------|
| D248767 | 0.11 | 0.23 | 0.23 | 0.34 | 0.69 | $k=2$ |
| D248763 | 0.13 | 0.36 | 0.23 | 0.45 | 0.90 | $k=2$ |

Key Comparison COOMET.QM-K120.b Carbon dioxide in Air

A1. General information

| | | | |
|----------------|---|-----|-----------------|
| Institute | Ukrmetrteststandart | | |
| Address | Metrologhichna str., 4; 03143 Kyiv; Ukraine | | |
| Contact person | OvsiyLevbarg | | |
| Telephone | +38044 526 5298 | Fax | +38044 526 3469 |
| Email* | molar@ukrcsm.kiev.ua | | |

A2. NMI submitted values

| | Cylinder Identification number | Carbon dioxide mole fraction $x_{\text{CO}_2, \text{cert}} / \mu\text{mol/mol}$ | Expanded uncertainty $U(x_{\text{CO}_2, \text{cert}}) / \mu\text{mol/mol}$ | Coverage factor |
|---|--------------------------------|--|---|-----------------|
| 1 | 81205102 | 480,27 | 0,45 | 2 |
| 2 | 81205166 | 799,99 | 0,83 | 2 |

A3. NMI submitted values

Matrix compositions: Component mole fractions and uncertainties (for each standard submitted):

(Standard 1) Cylinder Identification Number: **81205102**

| Component | Mole fraction value | Unit | Expanded uncertainty | Unit | Coverage factor |
|------------------|---------------------|---------------------|----------------------|---------------------|-----------------|
| N ₂ | 0,782774 | mol/mol | 0,000012 | mol/mol | 2 |
| O ₂ | 0,207361 | mol/mol | 0,000011 | mol/mol | 2 |
| Ar | 0,009382 | mol/mol | 0,000005 | mol/mol | 2 |
| CH ₄ | 91 | nmol/mol | 3 | nmol/mol | 2 |
| N ₂ O | not measured | nmol/mol | - | nmol/mol | - |
| CO | 77 | nmol/mol | 3 | nmol/mol | 2 |
| H ₂ O | 2,03 | $\mu\text{mol/mol}$ | 0,12 | $\mu\text{mol/mol}$ | 2 |

(Standard 2) Cylinder Identification Number: **81205166**

| Component | Mole fraction value | Unit | Expanded uncertainty | Unit | Coverage factor |
|------------------|---------------------|----------|----------------------|----------|-----------------|
| N ₂ | 0,781565 | mol/mol | 0,000011 | mol/mol | 2 |
| O ₂ | 0,208084 | mol/mol | 0,000011 | mol/mol | 2 |
| Ar | 0,009548 | mol/mol | 0,000004 | mol/mol | 2 |
| CH ₄ | 93 | nmol/mol | 3 | nmol/mol | 2 |
| N ₂ O | not measured | nmol/mol | - | nmol/mol | - |
| CO | 88 | nmol/mol | 3 | nmol/mol | 2 |
| H ₂ O | 2,26 | μmol/mol | 0,10 | μmol/mol | 2 |

CO₂ isotope ratio (vs. VPDB) for each standard submitted (Optional):

| | Cylinder Identification Number | δ ¹³ C | U(δ ¹³ C) | Coverage Factor | δ ¹⁸ O | U(δ ¹⁸ O) | Coverage Factor |
|---|--------------------------------|-------------------|----------------------|-----------------|-------------------|----------------------|-----------------|
| 1 | not measured | | | | | | |
| 2 | not measured | | | | | | |

A4. Uncertainty Budget

A combined standard uncertainty of the amount fraction of CO₂, $u_c(y_k)$, in the final mixtures was calculated using formula from ISO 6142-1:2015

$$u_c(y_k) = \frac{1}{2} \sqrt{u^2(y_{k, \text{prep}}) + u^2(y_{k, \text{ver}}) + (y_{k, \text{prep}} - y_{k, \text{ver}})^2}$$

where $u(y_{k, \text{prep}})$ is a gravimetric preparation standard uncertainty, $u(y_{k, \text{ver}})$ is a verification standard uncertainty, $y_{k, \text{prep}}$ and $y_{k, \text{ver}}$ are amount fraction values obtained by gravimetric procedure and by verification, respectively.

$y_{k, \text{prep}}$ and $u(y_{k, \text{prep}})$ were calculated according to the ISO 6142-1:2015 based on the transferred parent-gas masses with their uncertainties, as well as purity tables for parent gases and pre-mixture composition that are given below in A.5.

$y_{k, \text{ver}}$ and $u(y_{k, \text{ver}})$ were calculated according to ISO 6143:2001.

An expanded uncertainty, $U_c(y_k)$, was calculated as $U_c(y_k) = k \times u_c(y_k)$, where $k = 2$.

Uncertainty budget is given in the table:

| Cylinder Identification Number | $u(y_{k, \text{prep}})$, μmol/mol | $u(y_{k, \text{ver}})$, μmol/mol | $ y_{k, \text{prep}} - y_{k, \text{ver}} $, μmol/mol | $u_c(y_k)$, μmol/mol | $U_c(y_k)$, μmol/mol |
|--------------------------------|------------------------------------|-----------------------------------|---|-----------------------|-----------------------|
| 81205102 | 0,133 | 0,292 | 0,311 | 0,223 | 0,45 |
| 81205166 | 0,149 | 0,497 | 0,651 | 0,416 | 0,83 |

A5. Additional information

a) Purity table for CO₂

Purity table for CO₂

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|-------------------------------|---|--|-----------------|
| CO ₂ | 99,9885 | 0,0005 | 2 |
| N ₂ | 0,0082 | 0,0004 | 2 |
| O ₂ | 0,00020 | 0,00006 | 2 |
| CH ₄ | 0,00044 | 0,00002 | 2 |
| C ₂ H ₆ | 0,00045 | 0,00002 | 2 |
| H ₂ O | 0,0022 | 0,0001 | 2 |

b) Purity tables for other parent gases and pre-mixture composition

Purity table for N₂ (used to prepare pre-mixture)

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|------------------|---|--|-----------------|
| N ₂ | 99,9857 | 0,0008 | 2 |
| CO ₂ | 0,00047 | 0,00004 | 2 |
| O ₂ | 0,000019 | 0,000002 | 2 |
| CH ₄ | 0,000012 | 0,000001 | 2 |
| Ar | 0,0134 | 0,0007 | 2 |
| H ₂ O | 0,00037 | 0,00003 | 2 |

Purity table for N₂ (used to prepare Standard 1)

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|------------------|---|--|-----------------|
| N ₂ | 99,9866 | 0,0008 | 2 |
| CO | 0,000010 | 0,000001 | 2 |
| O ₂ | 0,000050 | 0,000005 | 2 |
| CH ₄ | 0,000010 | 0,000001 | 2 |
| Ar | 0,0133 | 0,0007 | 2 |
| H ₂ O | 0,00005 | 0,00001 | 2 |

Purity table for N₂ (used to prepare Standard 2)

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|-----------------|---|--|-----------------|
| N ₂ | 99,9930 | 0,0005 | 2 |
| CO | 0,000011 | 0,000001 | 2 |
| O ₂ | 0,000122 | 0,000006 | 2 |
| CH ₄ | 0,0000017 | 0,0000002 | 2 |
| Ar | 0,0068 | 0,0004 | 2 |

| | | | |
|------------------|---------|---------|---|
| H ₂ O | 0,00007 | 0,00001 | 2 |
|------------------|---------|---------|---|

Purity table for O₂

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|------------------|---|--|-----------------|
| O ₂ | 99,9992 | 0,0001 | 2 |
| CO ₂ | 0,0000093 | 0,0000005 | 2 |
| CH ₄ | 0,000005 | 0,000001 | 2 |
| H ₂ O | 0,00076 | 0,00004 | 2 |

Purity table for Ar

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|------------------|---|--|-----------------|
| Ar | 99,9995 | 0,0001 | 2 |
| N ₂ | 0,000105 | 0,000005 | 2 |
| CO ₂ | 0,000092 | 0,000004 | 2 |
| O ₂ | 0,000044 | 0,000002 | 2 |
| CH ₄ | 0,000001 | 0,000001 | 2 |
| H ₂ O | 0,000242 | 0,000006 | 2 |

Pre-mixture composition

| Component | Mole fraction, 10 ⁻² mol/mol | Expanded uncertainty, 10 ⁻² mol/mol | Coverage Factor |
|------------------|---|--|-----------------|
| CO ₂ | 5,019 | 0,001 | 2 |
| N ₂ | 94,9676 | 0,001 | 2 |
| O ₂ | 0,000028 | 0,000003 | 2 |
| CH ₄ | 0,000033 | 0,000003 | 2 |
| Ar | 0,0127 | 0,0007 | 2 |
| H ₂ O | 0,00046 | 0,00004 | 2 |

c) CO₂/N₂ pre-mixture of about 5 % CO₂ mole fraction was prepared. Detailed composition of the pre-mixture is given above. Then it was diluted with pure oxygen, argon and nitrogen to obtain Standard 1 and Standard 2.

Pure nitrogen from three different cylinders was used to prepare pre-mixture, Standard 1 and Standard 2.

d) The prepared mixtures were verified by comparison according to ISO 6143:2001. For this purpose two additional three-mixture sets, having the same matrix and CO₂ mole fraction close to Standard 1 and Standard 2, respectively, were prepared. The mixtures were compared using gas chromatograph with methanizer and FID detector. The calibration function was linear.

e) Cylinders pressure before shipment to VNIIM was 12,9 MPa in both cylinders.

Report of stability measurements after return of the cylinders

| Cylinder Identification Number | Pressure before shipment to VNIIM, MPa | Pressure after return from VNIIM, MPa | Final analysis date before shipment to VNIIM | Final analysis date after return from VNIIM |
|--------------------------------|--|---------------------------------------|--|---|
| 81205102 | 12,9 | 11,0 | 29.05.2019 | 14.07.2021 |
| 81205166 | 12,9 | 11,0 | 06.06.2019 | 08.07.2021 |

Stability was evaluated by comparison with newly prepared primary gas mixtures of similar composition (one for each mole fraction level) in accordance with ISO 16664 and ISO 6142-1. Comparison procedure used was "Single-point through origin calibration" according to ISO 12963.

Stability evaluation results are given in the table below.

| Cylinder Identification Number | Before shipment | | After return $\mu\text{mol/mol}$ | | Drift, $\mu\text{mol/mol}$ |
|--------------------------------|--|----------------------------------|--|----------------------------------|----------------------------|
| | CO ₂ mole fraction, $\mu\text{mol/mol}$ | $u_c(y_k)$, $\mu\text{mol/mol}$ | CO ₂ mole fraction, $\mu\text{mol/mol}$ | $u_c(y_k)$, $\mu\text{mol/mol}$ | |
| 81205102 | 480,27 | 0,223 | 481,03 | 0,379 | 0,76 |
| 81205166 | 799,99 | 0,416 | 801,00 | 0,368 | 1,01 |

According to the criterion stated in ISO 16664 ($D > 2$, where D is given by Formula (A.1) of ISO 16664:

$$D = \frac{|x_0 - x_1|}{\sqrt{u^2(x_0) + u^2(x_1)}} \quad),$$

the drift is significant

The evaluated drift was treated as an uncertainty due to instability, $u(y_{k,\text{stab}})$, and accounted for in the uncertainty budget by Formula (7) of ISO 6142-1:

$$u(y_{k,\text{prep}}) = \sqrt{u^2(y_{k,\text{grav}}) + u^2(y_{k,\text{stab}})}$$

Uncertainty budget re-evaluated according to Formulae (7) and (9) of ISO 6142-1 is given in the table below.

| Cylinder Identification number | $u(y_{k,\text{grav}})$, $\mu\text{mol/mol}$ | $u(y_{k,\text{stab}})$, $\mu\text{mol/mol}$ | $u(y_{k,\text{prep}})$, $\mu\text{mol/mol}$ | $u(y_{k,\text{ver}})$, $\mu\text{mol/mol}$ | $ y_{k,\text{prep}} - y_{k,\text{ver}} $, $\mu\text{mol/mol}$ | $u_c(y_k)$, $\mu\text{mol/mol}$ | $U_c(y_k)$, $\mu\text{mol/mol}$ |
|--------------------------------|--|--|--|---|--|----------------------------------|----------------------------------|
| 81205102 | 0,133 | 0,76 | 0,77 | 0,292 | 0,311 | 0,441 | 0,88 |
| 81205166 | 0,149 | 1,01 | 1,02 | 0,497 | 0,651 | 0,654 | 1,3 |

Thus, final submitted values are as following:

| | Cylinder Identification number | Carbon dioxide mole fraction $x_{\text{CO}_2, \text{cert}} / \mu\text{mol/mol}$ | Expanded uncertainty $U(x_{\text{CO}_2, \text{cert}}) / \mu\text{mol/mol}$ | Coverage factor |
|---|--------------------------------|--|---|-----------------|
| 1 | 81205102 | 480,3 | 0,9 | 2 |
| 2 | 81205166 | 800,0 | 1,3 | 2 |

Authors: S. Kisel, O. Levbarg, D. Melnyk, M. Rozhnov, S. Shpilnyi, S. Yakubov

Key Comparison CCQM- K120
Carbon dioxide in Air

Submission form CCQM- K120- R

Project name:CCQM- K120 (Carbon dioxide in air).

Comparison: Comparison of laboratories' preparation capabilities for Carbon dioxide in Air Standards.

Proposed dates: 09/2016 to 12/2017.

Coordinating laboratories:

Bureau International des Poids et Mesures
Chemistry Department
Pavillon de Breteuil
92312 Sevres Cedex, France.

NIST
100 Bureau Drive, Stop 8300,
Gaithersburg, MD 20899- 8300
US

Study Coordinator: Edgar Flores
BIPM Chemistry Department
Phone: +33 (0)1 45 07 70 92
Fax: +33 (0)1 45 34 20 21
email: edgar.flores@bipm.org

Return of the form:

Please complete and return the form preferably by email to edgar.flores@bipm.org

A1. General information

| | | | |
|----------------|--|-----|------------------|
| Institute | D.I. Mendeleev Institute for Metrology (VNIIM) | | |
| Address | 19 Moskovsky pr., St. Petersburg, 190005, Russia | | |
| Contact person | Leonid Konopelko | | |
| Telephone | +7 812 315 11 45 | Fax | +7 812 315 15 17 |
| Email* | fhi@b10.vniim.ru | | |

A2. Participation

| | |
|------------------------|--------|
| I am participating in: | Yes/No |
| CCQM- K120.a | Yes |
| CCQM- K120.b | Yes |

A3. NMI submitted values

Table 1

| | Cylinder Identification number | Carbon dioxide mole fraction $x_{CO_2, cert}$ / $\mu\text{mol/mol}$ | Expanded uncertainty $U(x_{CO_2, cert})$ / $\mu\text{mol/mol}$ | Coverage factor |
|---|--------------------------------|--|---|-----------------|
| 1 | M365601 | 380.20 | 0.11 | 2 |
| 2 | M365664 | 480.18 | 0.13 | 2 |
| 3 | M365707 | 800.73 | 0.19 | 2 |

Matrix compositions: Component mole fractions and uncertainties (for each standard submitted):

Table 2: (Standard 1) Cylinder Identification Number M365601

| Component | Mole fraction Value | Unit | Expanded Uncertainty* | Unit | CoverageFactor |
|------------------|---------------------|--------------------------|-----------------------|--------------------------|----------------|
| N ₂ | 78.1015 | 10 ⁻² mol/mol | 0.0013 | 10 ⁻² mol/mol | 2 |
| O ₂ | 20.9188 | 10 ⁻² mol/mol | 0.0013 | 10 ⁻² mol/mol | 2 |
| Ar | 0.9416 | 10 ⁻² mol/mol | 0.0005 | 10 ⁻² mol/mol | 2 |
| CH ₄ | 0.00000094 | 10 ⁻² mol/mol | 0.00000022 | 10 ⁻² mol/mol | 2 |
| N ₂ O | not measured | | | | |

Table 3: (Standard 2) Cylinder Identification Number M365664

| Component | Mole fraction Value | Unit | Expanded Uncertainty* | Unit | CoverageFactor |
|------------------|---------------------|--------------------------|-----------------------|--------------------------|----------------|
| N ₂ | 78.0928 | 10 ⁻² mol/mol | 0.0011 | 10 ⁻² mol/mol | 2 |
| O ₂ | 20.9270 | 10 ⁻² mol/mol | 0.0012 | 10 ⁻² mol/mol | 2 |
| Ar | 0.9322 | 10 ⁻² mol/mol | 0.0005 | 10 ⁻² mol/mol | 2 |
| CH ₄ | 0.00000096 | 10 ⁻² mol/mol | 0.00000022 | 10 ⁻² mol/mol | 2 |
| N ₂ O | not measured | | | | |

Table 4:(Standard 3) Cylinder Identification Number M365707

| Component | Mole fraction Value | Unit | Expanded Uncertainty* | Unit | Coverage Factor |
|------------------|---------------------|--------------------------|-----------------------|--------------------------|-----------------|
| N ₂ | 78.1000 | 10 ⁻² mol/mol | 0.0011 | 10 ⁻² mol/mol | 2 |
| O ₂ | 20.9199 | 10 ⁻² mol/mol | 0.0012 | 10 ⁻² mol/mol | 2 |
| Ar | 0.9000 | 10 ⁻² mol/mol | 0.0005 | 10 ⁻² mol/mol | 2 |
| CH ₄ | 0.00000097 | 10 ⁻² mol/mol | 0.00000022 | 10 ⁻² mol/mol | 2 |
| N ₂ O | not measured | | | | |

*Uncertainty in the tables 2-4 includes only constituents related to gravimetry (weighing and purity)

Table 5: CO₂ isotope ratio (vs. VPDB) for each standard submitted (Optional):

| | Cylinder Identification Number | $\delta^{13}\text{C}$ | $U(\delta^{13}\text{C})$ | Coverage Factor | $\delta^{18}\text{O}$ | $U(\delta^{18}\text{O})$ | Coverage Factor |
|---|--------------------------------|-----------------------|--------------------------|-----------------|-----------------------|--------------------------|-----------------|
| 1 | M365601 | -48.0 | 0.9 | 2 | - | - | - |
| 2 | M365664 | -48.0 | 0.9 | 2 | - | - | - |
| 3 | M365707 | -48.0 | 0.9 | 2 | - | - | - |

A4. Uncertainty Budget

Table 6: Uncertainty budget (only gravimetry) for CO₂ mole fraction for the cylinder M365601

| Uncertainty source X_i | | Estimate x_i | Evaluation type (A or B) | Distribution | Standard uncertainty $u(x_i)$ | Sensitivity coefficient c_i | Contribution $u_i(y)$ $\mu\text{mol/mol}$ |
|---|-----------------|--------------------------------|--------------------------|--------------|-------------------------------|-------------------------------|---|
| Purity of N ₂ | | 999998.672 $\mu\text{mol/mol}$ | B | Rectangular | 0.200 $\mu\text{mol/mol}$ | 0.00545 | 0.00109 |
| Purity of O ₂ | | 999999.381 $\mu\text{mol/mol}$ | B | Rectangular | 0.015 $\mu\text{mol/mol}$ | 0.06733 | 0.00101 |
| Purity of CO ₂ | | 999993.450 $\mu\text{mol/mol}$ | B | Rectangular | 0.374 $\mu\text{mol/mol}$ | 0.00016 | 0.00006 |
| Purity of Ar | | 999998.209 $\mu\text{mol/mol}$ | B | Rectangular | 0.030 $\mu\text{mol/mol}$ | 0.00534 | 0.00016 |
| Weighing** pre-mixture | CO ₂ | 20.15723g | A,B | Normal | 0.00223g | -18.54106 | -0.04140 |
| | N ₂ | 1153.59704g | A,B | Normal | 0.01962 g | 0.32397 | 0.00636 |
| Weighing** final mixture | pre-mixture | 20.48733 g | A,B | Normal | 0.00203 g | -17.91563 | -0.03630 |
| | Ar | 7.90915 g | A,B | Normal | 0.00200 g | 0.45258 | 0.00091 |
| | O ₂ | 140.75497 g | A,B | Normal | 0.00353 g | 0.56493 | 0.00200 |
| | N ₂ | 439.93136 g | A,B | Normal | 0.01021 g | 0.64543 | 0.00659 |
| Molar mass of CO ₂ (component due to isotopic composition) | | 44.0100 g/mol | A | Normal | 0.00035 g/mol | 8.6286 | 0.00302 |
| Combined standard uncertainty | | | | | | | 0.05596 |

| | |
|--------------------------|--------------|
| Expanded uncertainty k=2 | 0.112 |
|--------------------------|--------------|

Table 7: Uncertainty budget (only gravimetry) for CO₂ mole fraction for the cylinder M365664

| Uncertainty source X_i | Estimate x_i | Evaluati on type (A or B) | Distribution | Standard uncertainty $u(x_i)$ | Sensitivity coefficient c_i | Contribution $u_i(y)$ $\mu\text{mol/mol}$ | |
|---|--------------------------------|---------------------------------|--------------|-------------------------------------|-------------------------------------|---|----------|
| Purity of N ₂ | 999998.672 $\mu\text{mol/mol}$ | B | Rectangular | 0.200 $\mu\text{mol/mol}$ | 0.00545 | 0.00109 | |
| Purity of O ₂ | 999999.390 $\mu\text{mol/mol}$ | B | Rectangular | 0.011 $\mu\text{mol/mol}$ | 0.06909 | 0.00076 | |
| Purity of CO ₂ | 999993.450 $\mu\text{mol/mol}$ | B | Rectangular | 0.374 $\mu\text{mol/mol}$ | 0.00020 | 0.000075 | |
| Purity of Ar | 999998.209 $\mu\text{mol/mol}$ | B | Rectangular | 0.030 $\mu\text{mol/mol}$ | 0.00534 | 0.00016 | |
| Weighing** premixture | CO ₂ | 19.47854g | A,B | Normal | 0.00224g | -24.23572 | -0.05424 |
| | N ₂ | 1118.50932g | A,B | Normal | 0.01950 g | 0.42206 | 0.00823 |
| Weighing** final mixture | pre- mixture | 25.86420 g | A,B | Normal | 0.00204 g | -17.75177 | -0.03626 |
| | Ar | 7.80100 g | A,B | Normal | 0.00200 g | 0.57374 | 0.00115 |
| | O ₂ | 140.28618 g | A,B | Normal | 0.00391 g | 0.71611 | 0.00280 |
| | N ₂ | 432.88272 g | A,B | Normal | 0.00915 g | 0.81821 | 0.00749 |
| Molar mass of CO ₂ (component due to isotopic composition) | 44.0100 g/mol | A | Normal | 0.00035 g/mol | 10.9066 | 0.00382 | |
| Combined standard uncertainty | | | | | | 0.066379 | |
| Expanded uncertainty k=2 | | | | | | 0.133 | |

Table 8: Uncertainty budget (only gravimetry) for CO₂ mole fraction for the cylinder M365707

| Uncertainty source X_i | Estimate x_i | Evaluati on type (A or B) | Distribution | Standard uncertainty $u(x_i)$ | Sensitivity coefficient c_i | Contributio n $u_i(y)$ $\mu\text{mol/mol}$ | |
|-----------------------------|--------------------------------|---------------------------------|--------------|-------------------------------------|-------------------------------------|---|----------|
| Purity of N ₂ | 999998.672 $\mu\text{mol/mol}$ | B | Rectangular | 0.200 $\mu\text{mol/mol}$ | 0.00545 | 0.00109 | |
| Purity of O ₂ | 999999.390 $\mu\text{mol/mol}$ | B | Rectangular | 0.011 $\mu\text{mol/mol}$ | 0.06733 | 0.00076 | |
| Purity of CO ₂ | 999993.450 $\mu\text{mol/mol}$ | B | Rectangular | 0.374 $\mu\text{mol/mol}$ | 0.00035 | 0.00013 | |
| Purity of Ar | 999998.209 $\mu\text{mol/mol}$ | B | Rectangular | 0.030 $\mu\text{mol/mol}$ | 0.00500 | 0.00015 | |
| Weighing** premixture | CO ₂ | 20.15723 g | A,B | Normal | 0.00223g | -39.05886 | -0.08721 |
| | N ₂ | 1153.59704g | A,B | Normal | 0.01962 g | 0.68249 | 0.01339 |

| | | | | | | | |
|---|-----------------|---------------|-----|--------|---------------|-----------|----------------|
| Weighing** final mixture | pre- mixture | 42.82195 g | A,B | Normal | 0.00220 g | -17.33744 | -0.03823 |
| | Ar | 7.50252 g | A,B | Normal | 0.00202 g | 0.96046 | 0.00194 |
| | O ₂ | 139.69676 g | A,B | Normal | 0.00403 g | 1.19851 | 0.00483 |
| | N ₂ | 414.48867 g | A,B | Normal | 0.00834 g | 1.36969 | 0.01143 |
| Molar mass of CO ₂ (component due to isotopic composition) | | 44.0100 g/mol | A | Normal | 0.00035 g/mol | 18.1777 | 0.006362 |
| Combined standard uncertainty | | | | | | | 0.09719 |
| Expanded uncertainty k=2 | | | | | | | 0.194 |

**Uncertainty due to weighing includes constituents related to accuracy of balance, buoyancy effect resulting from change of cylinder volume during filling, mass pieces used, drift of balance, residual gas in cylinder.

A5. Additional information

Table 9: Purity table with uncertainties for the nominally pure CO₂ parent gas

| Cylinder N 74318 Main component CO ₂ Mole fraction 99.999345% | | |
|--|------------------------------------|---|
| Component | Mole fraction, $\mu\text{mol/mol}$ | Standard uncertainty, $\mu\text{mol/mol}$ |
| N ₂ | 0.25 | 0.14 |
| CO | 0.029 | 0.001 |
| CH ₄ | 0.149 | 0.002 |
| He | 0.5 | 0.29 |
| H ₂ | 3.22 | 0.07 |
| O ₂ | 0.25 | 0.14 |
| H ₂ O | 2.15 | 0.11 |

Purity tables with uncertainties for the nominally pure N₂, O₂, and Ar parent gases

Table 10: Purity table for N₂

| Monoblock Main component N ₂ Mole fraction 99.9998672% | | |
|---|------------------------------------|---|
| Component | Mole fraction, $\mu\text{mol/mol}$ | Standard uncertainty, $\mu\text{mol/mol}$ |
| Ar | 0.916 | 0.011 |
| O ₂ | 0.0015 | 0.0009 |
| CO ₂ | 0.0025 | 0.0014 |
| H ₂ | 0.0025 | 0.0014 |
| CH ₄ | 0.0025 | 0.0014 |
| CO | 0.0025 | 0.0014 |
| H ₂ O | 0.40 | 0.20 |

Table 11: Purity table for O₂

| Cylinder N 910281 | | |
|--|-------------------------|--------------------------------|
| Main component O ₂ Mole fraction 99.9999381% | | |
| Component | Mole fraction, μmol/mol | Standard uncertainty, μmol/mol |
| H ₂ | 0.0025 | 0.0014 |
| Ar | 0.181 | 0.004 |
| N ₂ | 0.307 | 0.012 |
| Kr | 0.0025 | 0.0014 |
| CO | 0.0075 | 0.0043 |
| CH ₄ | 0.0347 | 0.0008 |
| CO ₂ | 0.081 | 0.005 |
| Xe | 0.0025 | 0.0014 |

Table 12: Purity table for Ar

| Cylinder N 283162 | | |
|---|-------------------------|--------------------------------|
| Main component Ar Mole fraction 99.9998209% | | |
| Component | Mole fraction, μmol/mol | Standard uncertainty, μmol/mol |
| O ₂ | 0.0231 | 0.0013 |
| N ₂ | 1.188 | 0.015 |
| CH ₄ | 0.015 | 0.009 |
| CO ₂ | 0.030 | 0.017 |
| H ₂ | 0.025 | 0.014 |
| CO | 0.010 | 0.006 |
| H ₂ O | 0.50 | 0.01 |

c) a brief outline of the dilution series undertaken to produce the final mixtures

Preparation of final mixtures (CO₂ in synthetic air) was carried out from pure substances in 2 stages:

1-st stage – 3 mixtures CO₂/N₂ –level 1.1 %,

2-nd stage – 3x3 target mixtures CO₂/synthetic air.

All the mixtures were prepared in Luxfer cylinders (V=10 and 5 dm³)

d) a brief outline of the verification procedure applied to the final mixtures;

CRDS analyzer was used for verification

4 measurement series were carried out within each verification procedure.

SD of a single measurement (reproducibility between series) was 0,003 % -0,006 %.

CRDS analyzer was used for verification

Instrument: Picarro G2401

Measurement cell temperature: 45°C

Measurement cell pressure: 18,665 kPa

Data collection: by "Picarro Inc." software

CRDS analyzer was used for δ¹³C measurements

Instrument: Picarro G2131i

Reference materials used for calibration: IAEA-CO-8, IAEA-CH-7

Measurement cell temperature: 45°C

Measurement cell pressure: 18,665 kPa
Data collection: by "Picarro Inc." software

e) a brief outline of any stability testing of the mixtures between the time they are prepared and the time they are shipped to the BIPM

The final mixtures were prepared 03.10 -13.10.2016.

First verification measurement was carried out 17.10 -21.10 2016.

Second verification measurement was carried out 26.10 -28.10.2016.

Verification measurements were performed by checking consistency within the group of the 3x3 prepared mixtures.

$u_{ver} = 0,003 \%$

Stability testing (short-term) did not show instability within the accuracy of the measurement method.

Long-term stability testing (measurements 21.08.-23.08.2017 and 09.10-11.10.2017) did not show instability within the accuracy of the measurement method.

f) cylinder pressure before shipment to the BIPM

8.9 MPa for M365601

9.0 MPa for M365664

9.3 MPa for M365707